

Difference of Electrical Impedance between Typical Benign Prostatic Hyperplasia Tissues and Beach Balls Retrieved after Holmium Laser Enucleation of the Prostate

Kim HW¹, Yun J², Shin DG¹, Lee W³, Choi S⁴, Yoon CS⁵, Oh TH⁶, Cho WY⁷, Chung MK⁸, Lee J¹, Lee JZ¹

1. Pusan National University Hospital, 2. Gwangju Institute of Science and Technology, 3. Dongnam Institute of Radiology and Medical Science, 4. Kosin University College of Medicine, 5. BHS Han-seo Hospital, 6. Samsung Changwon Hospital, 7. Dong-A University Hospital, 8. Pusan National University Yangsan Hospital

BACKGROUND

[Electrical Impedance]

- A measure of total resistance to alternating current, and is defined in the frequency domain (Hz).
- Because the electrical properties of tissues are closely related to their physical and physiological states, different impedance is measured from different type of tissues.

[Electrical impedance spectroscopy (EIS)]

- Sensitively characterizes different type of tissues in terms of impedance.

[EIS-on-a-Needle (EoN)]

- EIS added on a hypodermic needle.
- Can analyze the impedance of tissues in the frequency domain.

OBJECTIVES

- Different pathologic features between **typical benign prostatic hyperplasia (BPH) tissues** and **beach balls** which are retrieved after Holmium Laser Enucleation of the Prostate (HoLEP) may affect the electrophysiological characteristics of the two types of the tissues.
- To investigate the difference of **electrical impedance** between the two types of prostatic tissues, our group has developed a needle sensor device by incorporating EIS sensor on a tip of a hypodermic needle, which we named "EoN".

MATERIALS & METHODS

[Experimental process]

- Prostatic tissue samples from 10 patients who presented beach balls during morcellation after HoLEP were collected.
- A total of 10 respective pieces of **typical BPH tissues** and **beach balls** were prepared for the study by randomly selecting one piece of each type of tissues from each patients.
- **EoN** was fabricated by using the microelectromechanical system technology (Fig. 1a-c) and was connected to an impedance analyzer to measure the impedance of the tissues.
- The impedance of the samples was measured at the frequency range from 100 Hz to 1 MHz by inserting EoN at the depth of 2 mm into the tissues.
- Once the impedance of the samples were measured, they were pathologically investigated.

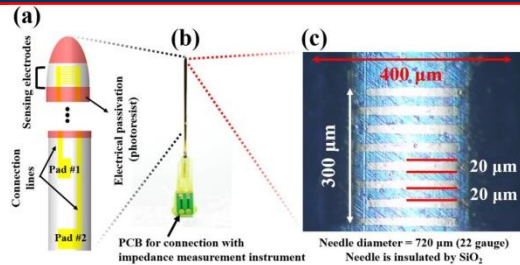


Fig 1. Schematic design of EoN.

[Data analysis]

- The **mean magnitude of impedance** between typical BPH tissues and beach balls at each frequencies between 100 Hz and 1 MHz were **compared**, and the degree of correlation between the magnitude and frequency in each type of tissues were evaluated.
- Also, the **variations of magnitude according to the frequency** were compared between the two types of prostatic tissues.

RESULTS

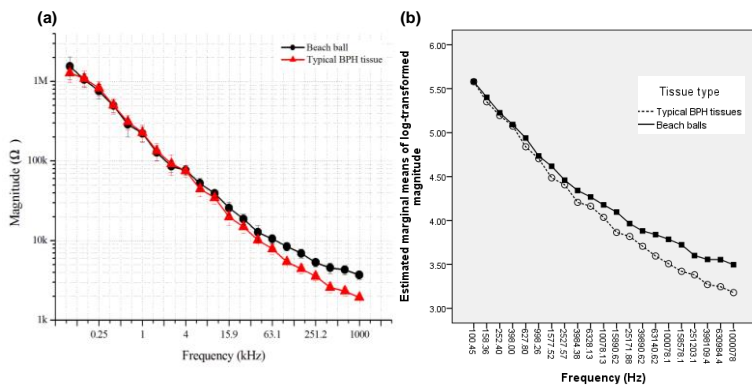


Fig 2. Results of comparison analysis between typical BPH tissues and beach balls.

[Results]

- The **mean magnitude** of the **beach balls** were tended to be **larger** than that of the typical BPH tissues at all frequencies from 100 Hz to 1 MHz (Fig 2a).
- Notably, **significantly larger mean magnitudes** were measured in the **beach balls** compared to the typical BPH tissues at the frequencies **higher than 15.9 kHz** ($p < 0.02$) at all frequencies higher than 15.9 kHz).
- Also, a **significant negative correlation** was presented between the measured **magnitudes** and **frequencies** in beach balls ($p < 0.001$) and typical BPH tissues ($p < 0.001$) which the correlation coefficient (r) was calculated as -0.28 and -0.29 , respectively.
- When the measured magnitude of the tissues were log-transformed, the **variation of mean log-transformed magnitudes according to the frequency** was **significantly different** between the two types of prostatic tissues ($p < 0.001$, Fig 2b).
- The pathologic features of the **beach balls** presented **pure stromal nodule of nodular hyperplasia** (consisted of only stroma) while the **typical BPH tissues** presented **mixed epithelial-stromal nodule of nodular hyperplasia** (composed of stroma + epithelium) (Fig 3).

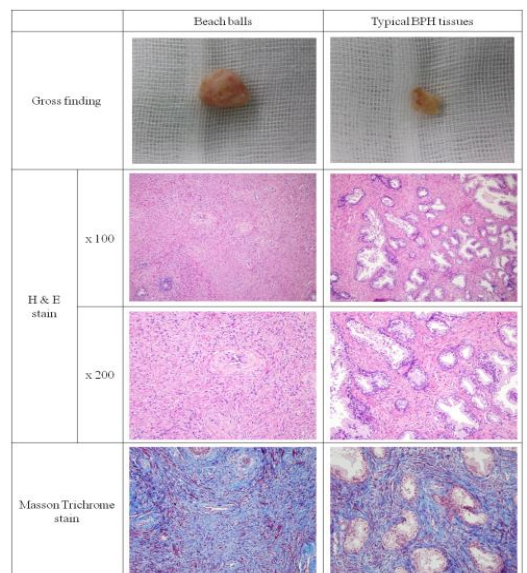


Fig 3. Gross and histologic findings of typical BPH tissues and beach balls.

[Interpretation of the results]

- **EoN** could **differentiate** between the two types of the prostatic tissues by comparing not only their **magnitude** of impedance, but also their **variation of log-transformed magnitude** according to the frequency.
- The significant difference regarding the magnitude of impedance between the typical BPH tissues and beach balls is assumed to be **affected by the difference of their pathological characteristics**.
- Since the beach balls have more abundant stromal content compared to the typical BPH tissues, its **larger mean magnitude of impedance is likely to be attributed by a larger amount of stroma** contained in the tissues.
- Such results imply that **the amount of stromal content affects the absolute value of impedance among the same type of tissues**.

CONCLUSION

- The needle device with EIS sensor could effectively discriminate between the typical BPH tissues and the beach balls by measuring their electrical impedance.
- The difference of impedance between the two types of prostatic tissues is assumed to be attributed by the amount of stromal content in the tissues.

DISCLOSURES STATEMENT

No competing financial interests exist.